

FIG. 2

TRANSMITTED LIGHT BASE

FIG. 2

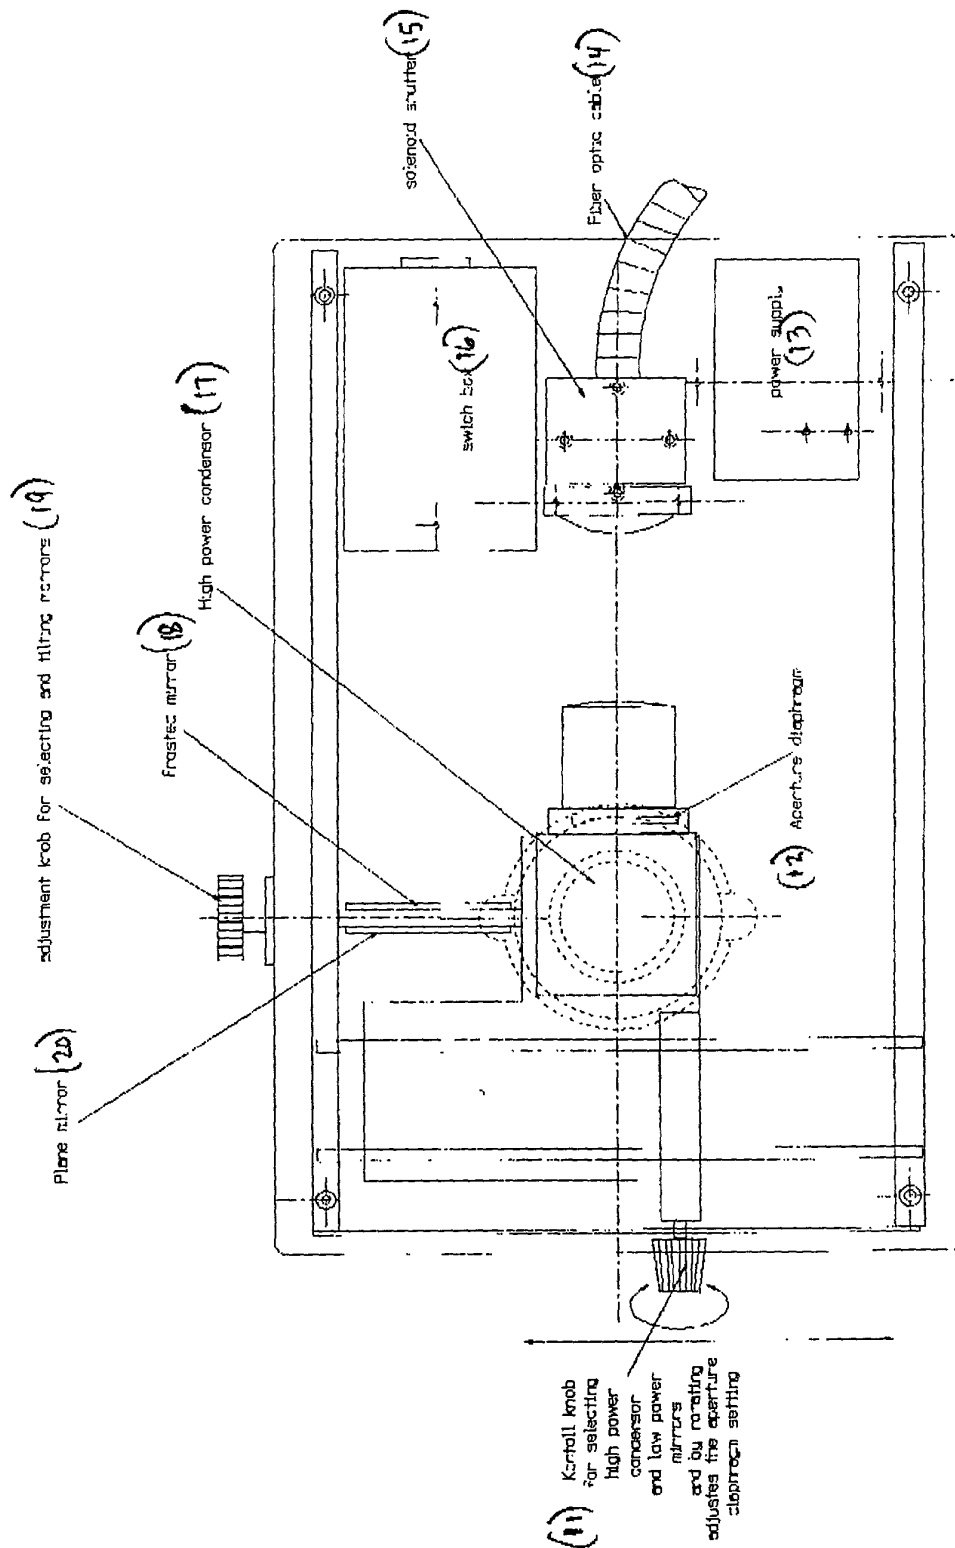
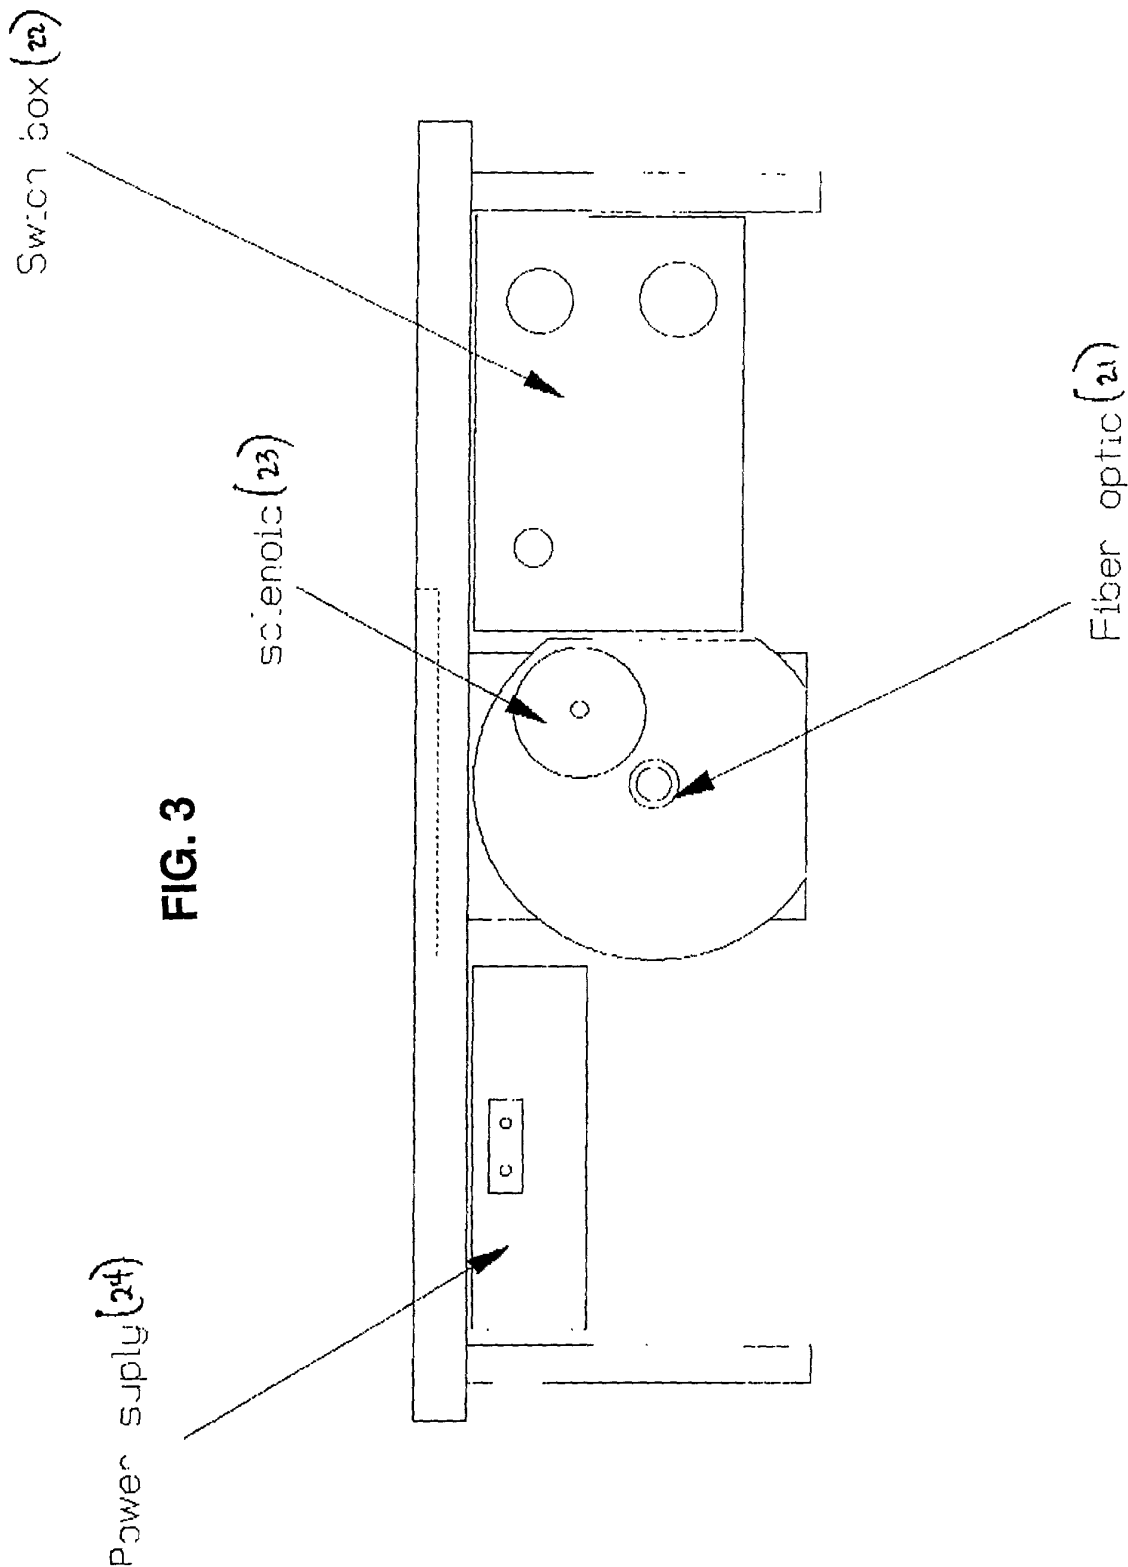


FIG. 3




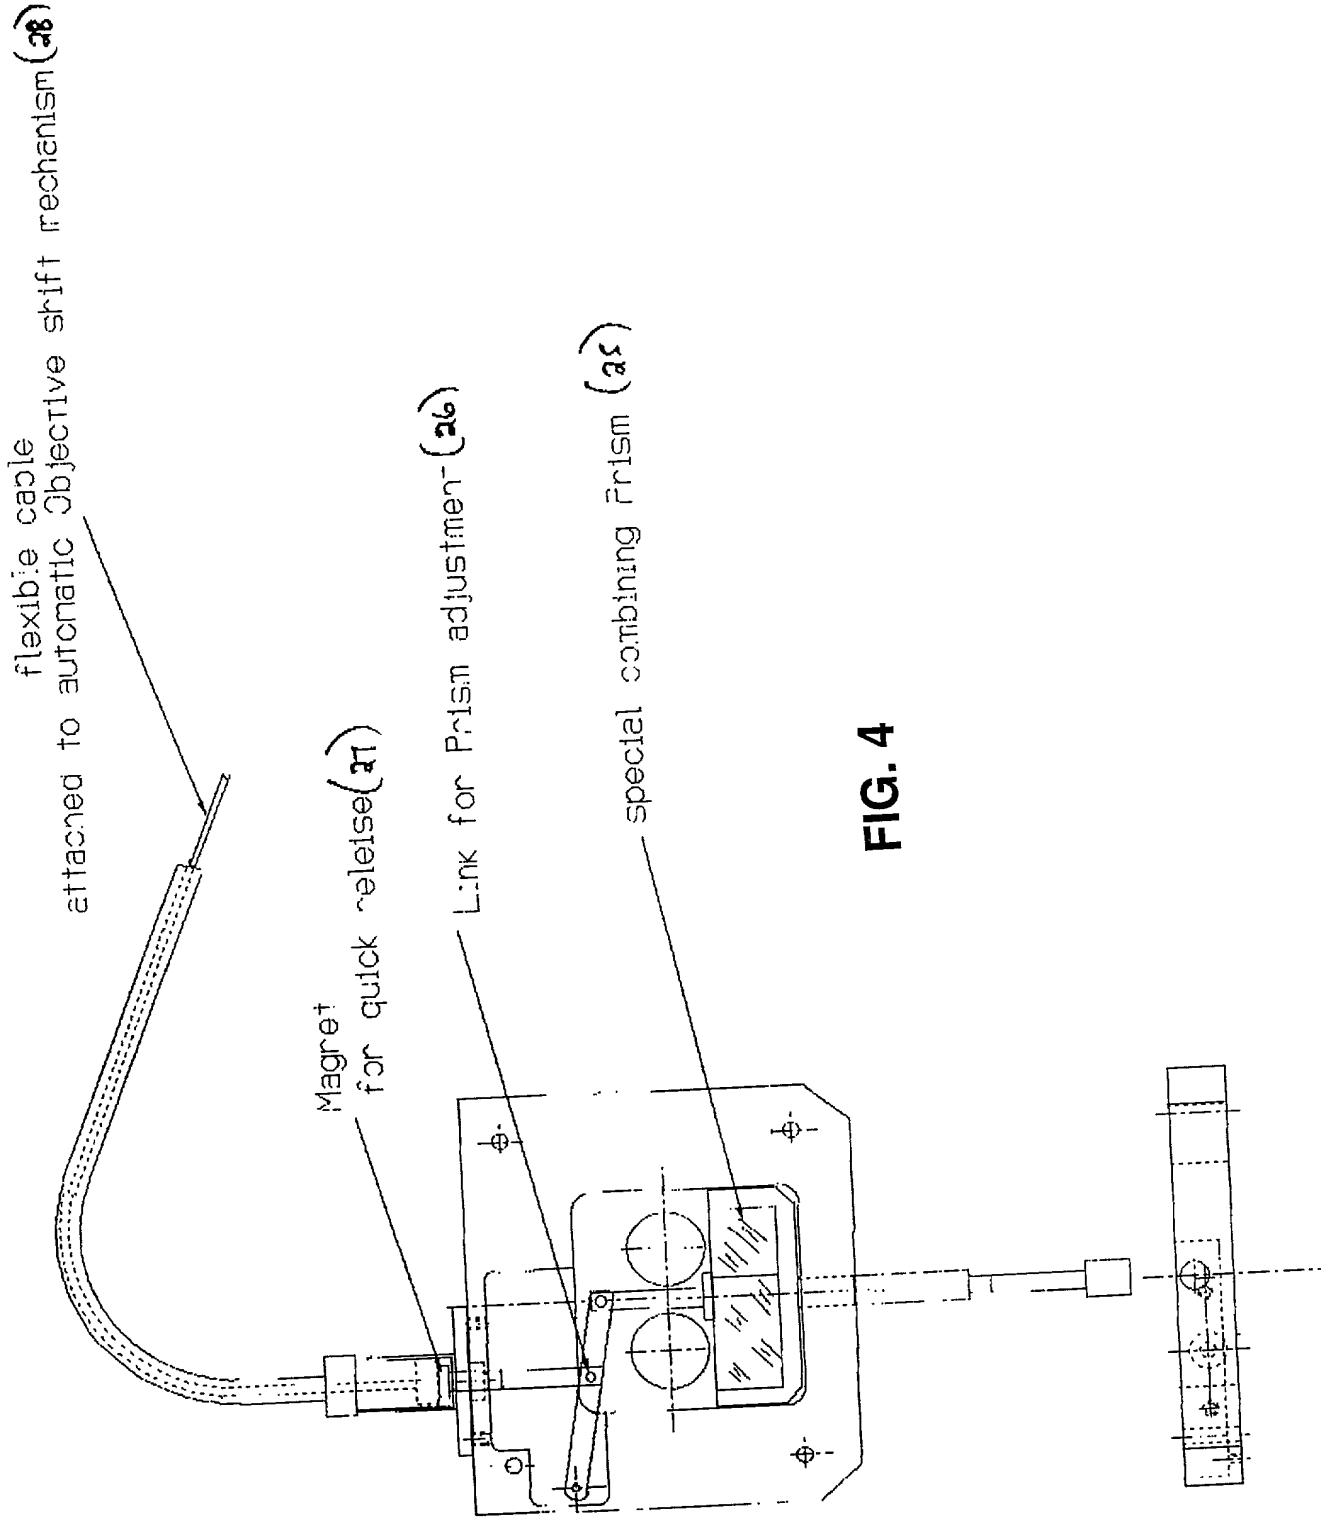


FIG. 4

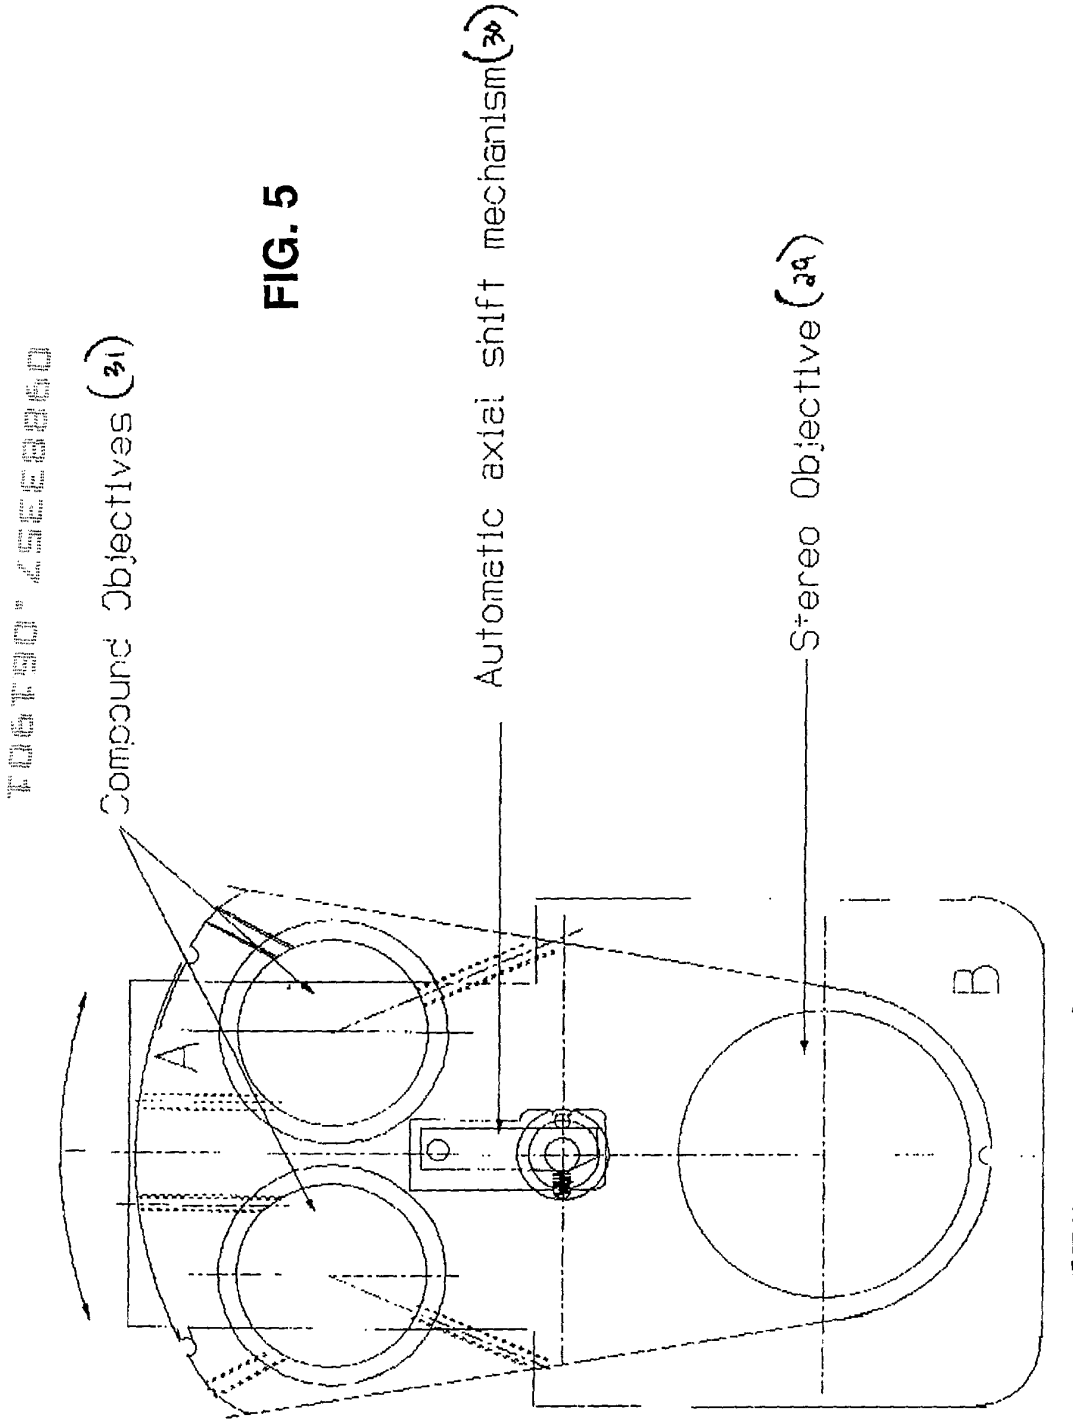

When rotating Objective nosepiece [A] the Microscope carrier [B] automatically moves from the Stereo Objective to the compound Objective position

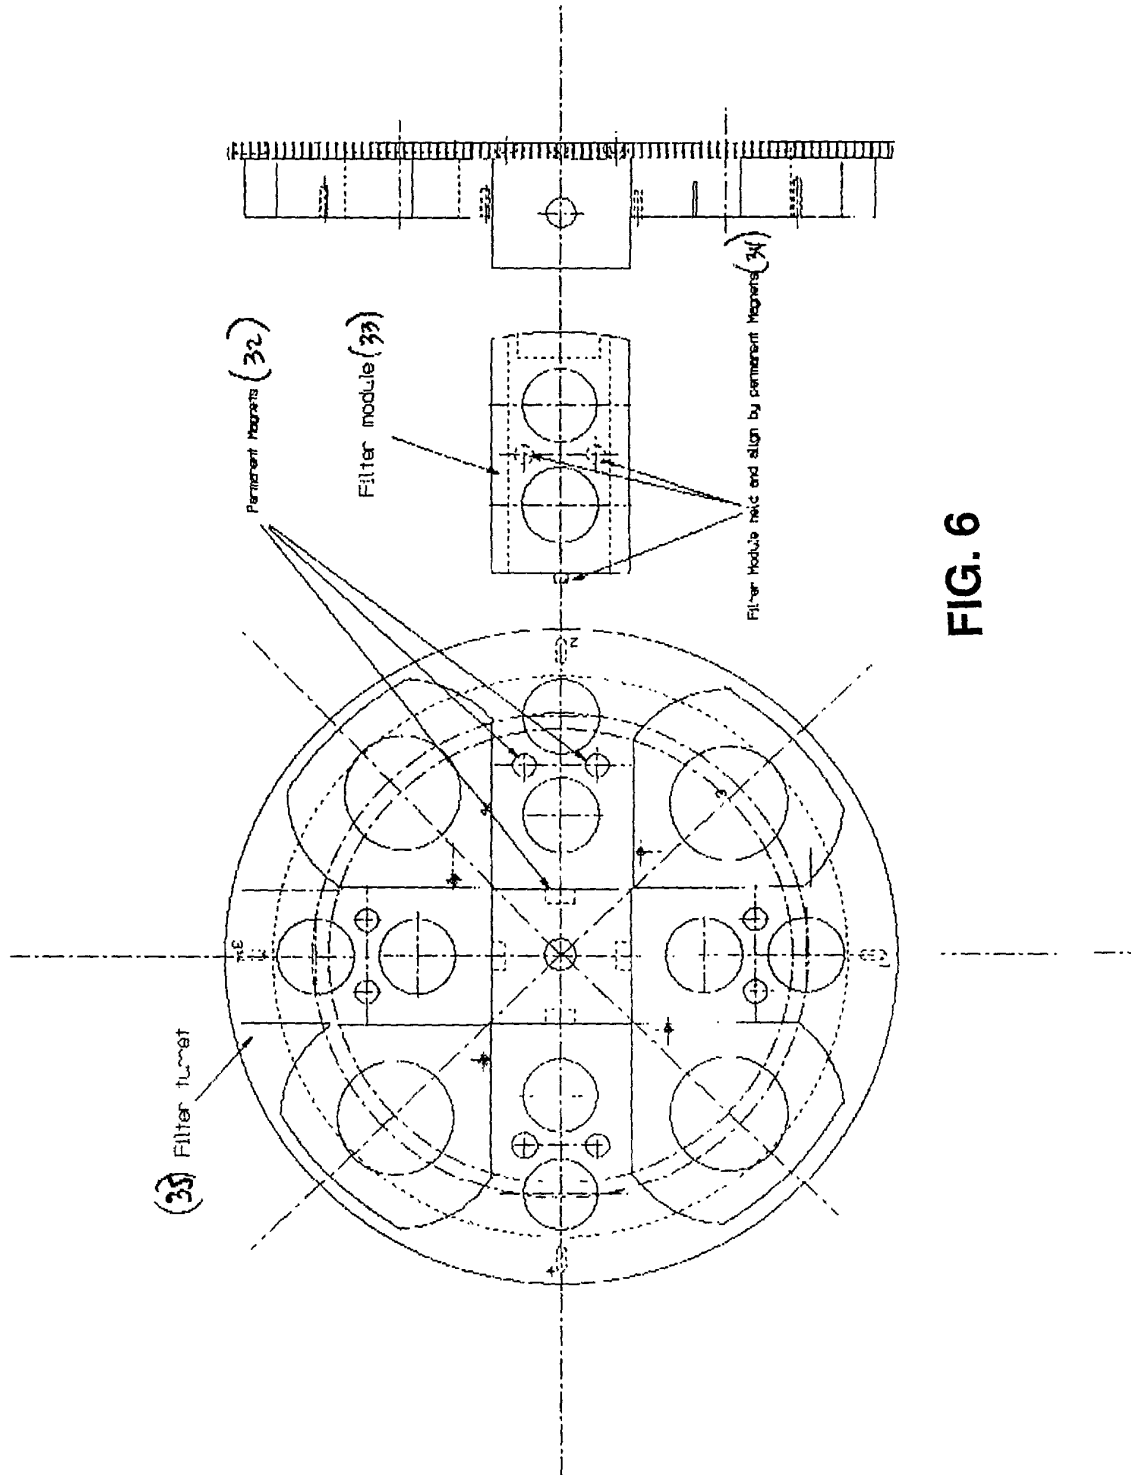


FIG. 6

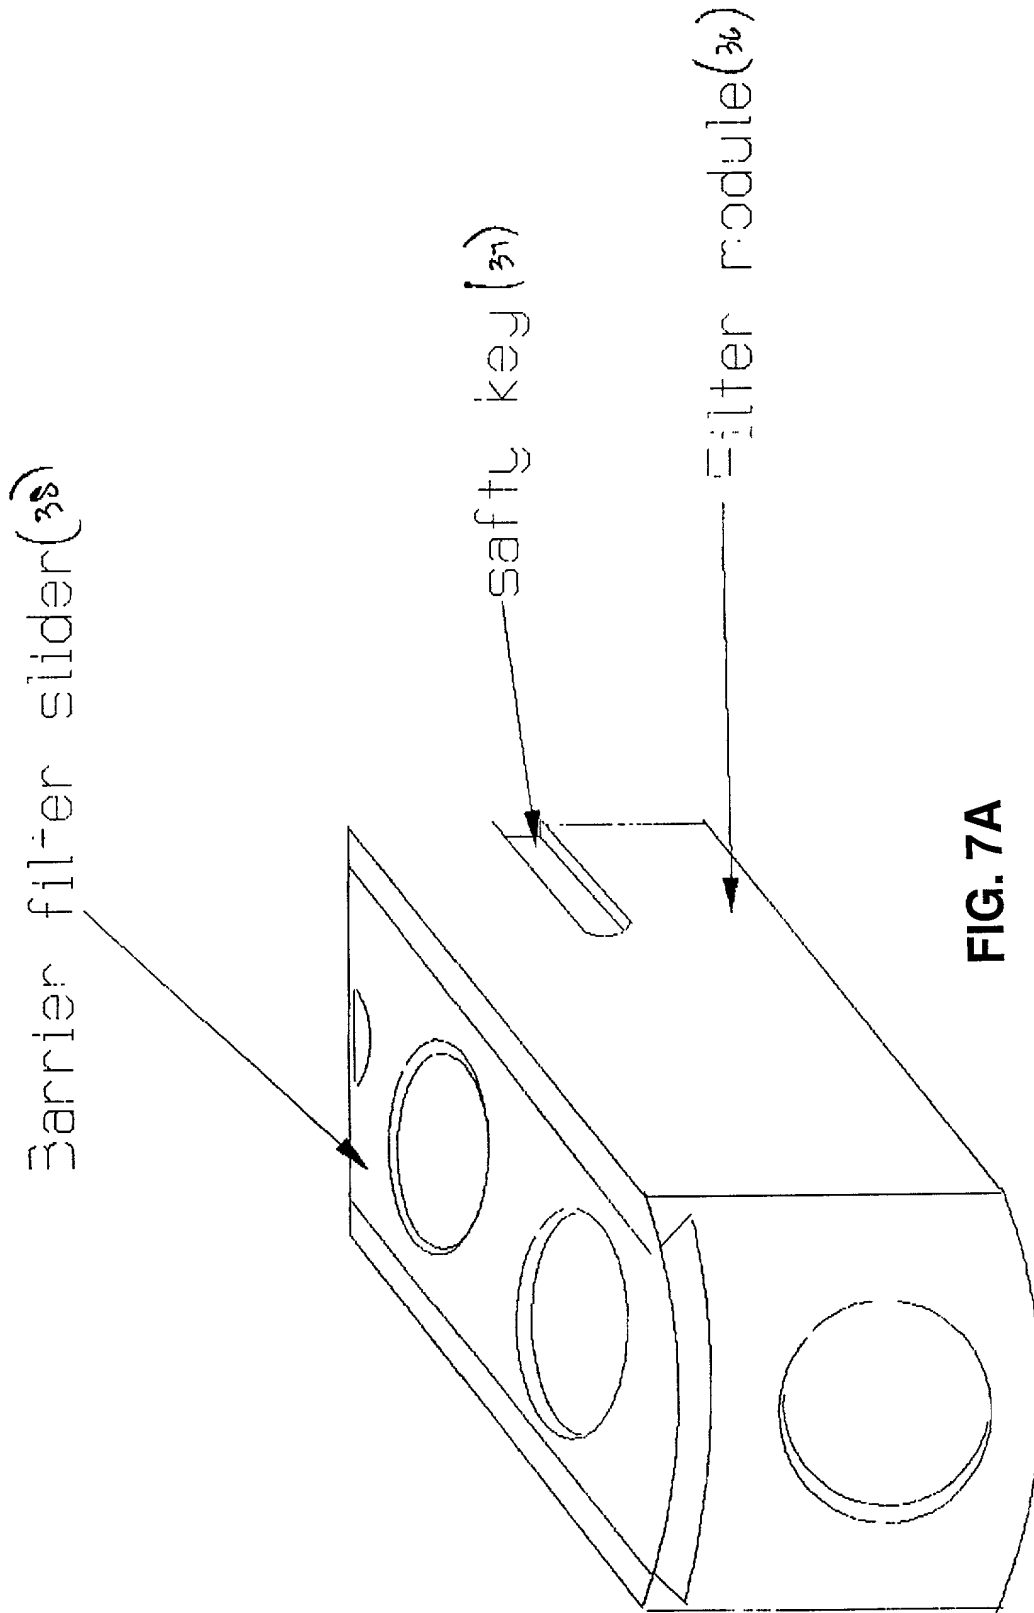


FIG. 7A

